

# Protein A ELISA

Instruction Manual  
for samples with or without IgG



IgY Lab Systems AB

[www.igylabs.com](http://www.igylabs.com)

## Table of content


1.	Background .....	2
2.	Assay principle.....	4
3.	Kit contents .....	5
4.	Materials not provided .....	6
5.	Precautions .....	6
6.	Reagent preparation .....	7
7.	Sample and standard preparation .....	8
8.	Test procedure.....	10
9.	Analysis of results .....	12
10.	Performance .....	13
11.	Tips and hints .....	16
12.	Related products.....	16
13.	References.....	17
14.	Quick start guide, samples without IgG .....	18
15.	Quick start guide, samples with IgG .....	19
16.	Contact and order information .....	20

---

## 1. Background

### 1.1 Staphylococcal Protein A (SpA)

SpA is an immunoglobulin (IgG)-binding protein found in the bacterial cell wall of *Staphylococcus aureus* (ref 1). SpA binds to most mammalian IgG and can be used for detection or purification of such antibodies (ref 2). Affinity chromatography on SpA columns is widely used for the purification of monoclonal and polyclonal antibodies. SpA may sometimes leak from the column and contaminate the preparation which may give false results in immunological assays. In the in vivo

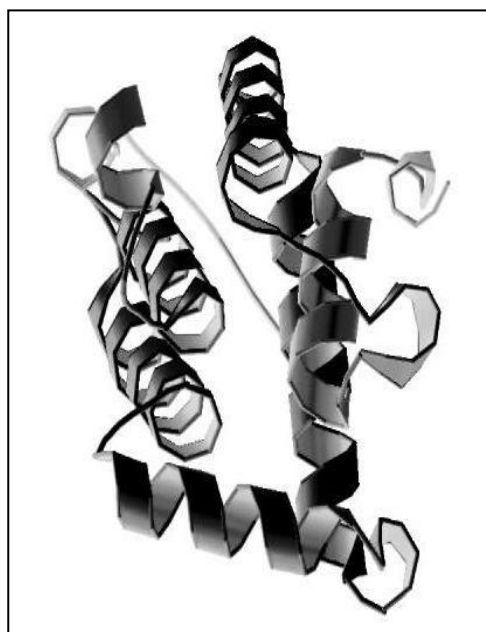


setting, SpA can react with IgG causing anaphylactic reactions (ref 1). Thus, it is important that antibody preparations are free from SpA before being used.

This kit has been developed and is primarily tested with recombinant SpA from GE Healthcare, which is also the source of the included SpA reference. Native SpA and other sources of recombinant SpA generally give good recoveries, but in some cases it may be necessary to use the same SpA source for the standard as for the samples being analysed.

## 1.2 Non-specific interactions between SpA and IgG

Analysing for the presence of SpA in samples containing IgG involves two major problems which must be overcome in order to obtain reliable results.

- **Fc binding.** SpA reacts with the Fc region of IgG from most animal species which makes its specific detection by immunoassay difficult. Antibodies specific for SpA will bind specifically as well as non-specifically due to the Fc reactivity of SpA. In this kit, the problem is solved by using chicken anti-SpA IgY. Chicken antibody is one of the few immunoglobulins that does not bind SpA in the Fc region.

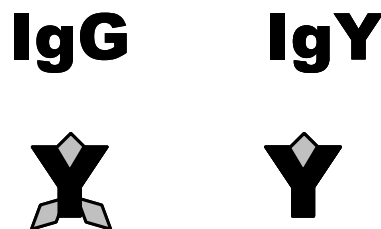


IgG binds SpA nonspecifically in the Fc region.  
This problem is overcome using chicken IgY  
since it is not Fc reactive to SpA.

- **Other non-specific interactions.** In samples containing mammalian IgG, immunologically active epitopes of SpA can be blocked by non-specifically bound IgG. To overcome this problem, SpA can be analysed at low pH (ref 4) since this should cause SpA and IgG to dissociate. However, high affinity antibodies (e.g. human IgG and certain mouse monoclonals) bind to SpA even below pH 3. Unfortunately, the specific immunological detection of SpA is very difficult at such low pH and an assay at this pH would likely have an unsatisfactory analytical performance. Instead, we have chosen to establish a flexible assay

system that can be tailored to each customer's situation. The standard references are made with known amounts of IgG present. The IgG solution, which is added to the standard references, should be as similar as possible to the IgG found in the samples. To dissociate SpA and IgG, the samples and standard references are boiled for 4 minutes. In other words, the assay is standardised with the same IgG that is present in the samples. The possible error from the blocking of antigenic epitopes is therefore eliminated.

## **2. Assay principle**

This ELISA kit is designed to detect SpA in IgG-containing solutions (e.g. monoclonal antibody preparations), in acid eluates from SpA columns, or in other liquid preparations. It is a sandwich ELISA based on microtitre strips precoated with the primary antibody, affinity-purified chicken anti-SpA. SpA from the sample is bound to the microwell and detected by biotinylated chicken anti-SpA antibody. Next, a streptavidin horseradish peroxidase conjugate is bound to the biotin conjugate. Finally, the substrate is added and reacts with the horseradish peroxidase to produce a colour change. Colour development indicates a positive result, and the colour can be read visually or by a microplate spectrophotometer at 450 nm. Samples to be tested with this assay are often of acidic pH. In order for the test to work properly, such samples should be neutralised. If a sample contains mammalian IgG, SpA may interact with the IgG and be partially blocked, falsely lowering the signal. To avoid this problem, samples containing IgG are treated to denature the IgG and expose SpA epitopes. A schematic outline of the assay is shown below.

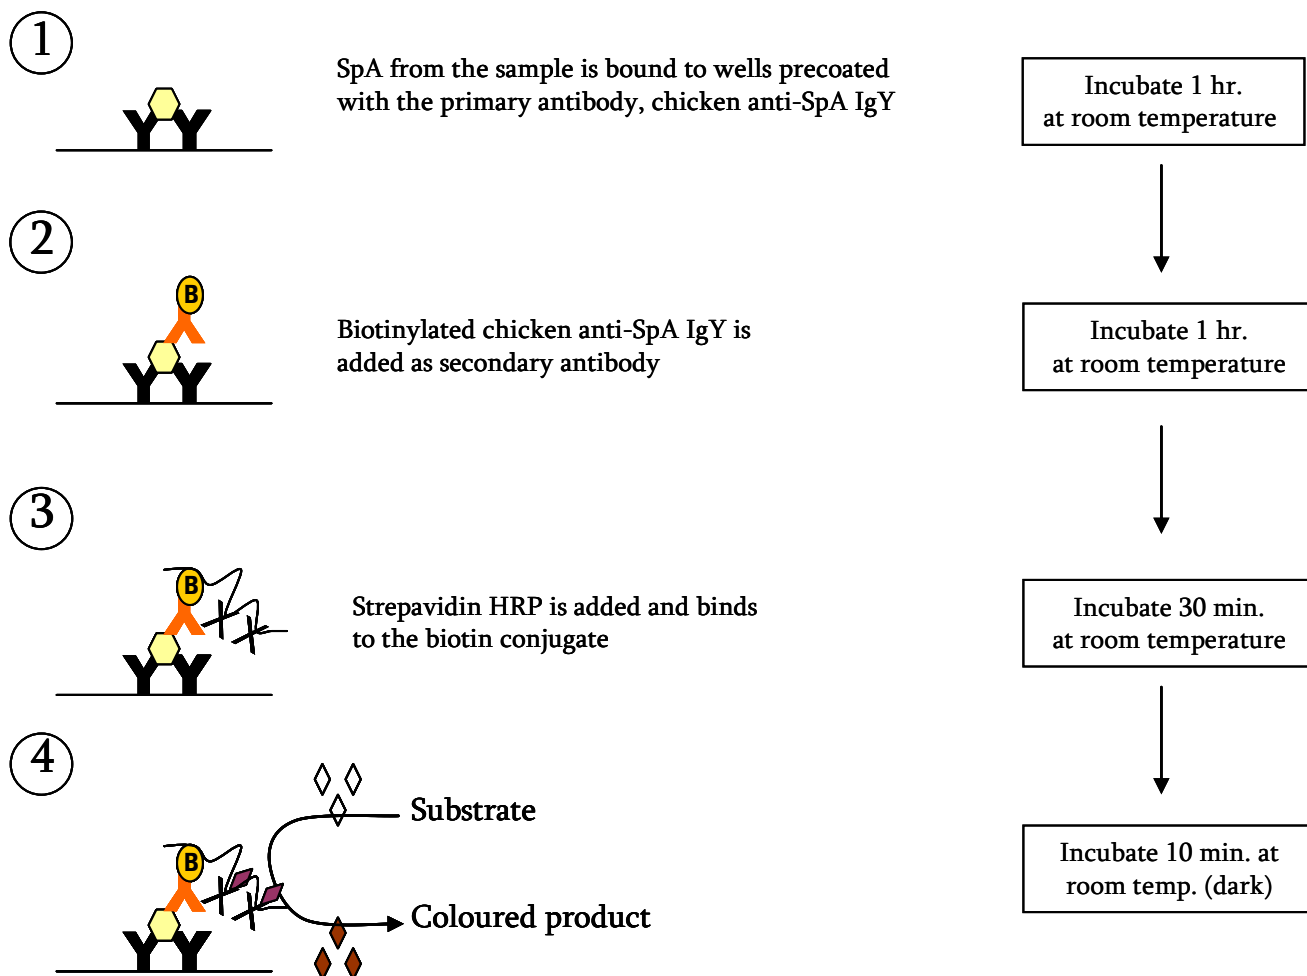

Substrate is added and reacts with HRP to produce a coloured product. Finally, stop solution is added to stop the chromogenic reaction.

### 3. Kit contents

- **Microtitre strips 8x12**, pre-coated with chicken anti-SpA antibody.
- **Wash tablets**, 3 tablets. Sufficient for 3x0.5 L Phosphate Buffered Saline with 0.1% Tween.
- **Protein A reference**, 200  $\mu$ L. 0.5 mg/mL SpA solution (recombinant origin). Contains preservative.
- **Tween 20 concentrate**, 3 mL.
- **Stop solution**, 25 mL. 1 M HCl. (Caution: Strong Acid)
- **Substrate solution**, 25 mL. TMB/H<sub>2</sub>O<sub>2</sub> solution.
- **HRP Conjugate**, 200  $\mu$ L. Streptavidin horseradish peroxidase conjugate. 100x solution. Contains preservative.
- **Biotinylated anti-SpA IgY**, 200  $\mu$ L. 100x solution. Contains preservative.
- **2 M Tris Buffer**, 25 mL.

## 4. Materials not provided

- Pipettes: 10 to 1,000  $\mu\text{L}$
- Microplate spectrophotometer
- Disposable pipette tips
- Eppendorf tubes
- 10-mL tubes
- Ultra pure water

Additional material needed to assay samples with IgG:

- SpA-free IgG solution
- Water bath
- Centrifuge (2000g)
- Vial rack or floating aid

## 5. Precautions

- Carefully read and follow all instructions.
- Store the kit and all reagents at +2 to +8°C (35 to 45°F).
- All reagents should equilibrate to room temperature +18 to +25°C (64 to 77°F) before use.
- Unused microtitre wells should be stored sealed at +2 to +8° C.
- Do not mix components or instruction booklets from kits with different expiration dates (different batches).
- Do not eat, drink, or smoke where specimens or kit reagents are handled.
- Do not use the kit beyond expiration date.
- This kit is for research use only.
- Use a separate pipette tip for each sample.
- Do not pipette by mouth.
- Standard references must be used for each new test series.
- Use only ultra pure water for preparation of reagents.
- The Substrate solution and 2 M Tris buffer are irritating to eyes, respiratory system and skin. Avoid contact with skin and eyes.
- The Stop solution contains HCl. This is a strong acid that can cause burns. Handle with care.
- Be careful to prevent contamination of kit components.

## 6. Reagent preparation

The examples below calculate the approximate amount needed to assay 96 microtitre wells (i.e. 12 strips). The amount of Neutralisation and Dilution buffer needed depends on the pH and concentration of the samples and therefore varies with each test.

- **Microtitre wells, Substrate solution and Stop solution** are ready for use.
- **Protein A reference.** Should be diluted according to step 7.4.
- **Tween solution.** Prepare Tween solution by diluting the concentrate 1:5 in ultra pure water. Example: Mix 1 mL Tween concentrate with 4 mL water. Vortex.
- **Neutralisation buffer.** Prepare by diluting Tween solution 1:5 in Tris Buffer. Example: Mix 1 mL Tween solution with 4 mL Tris buffer. Vortex.
- **Dilution buffer.** Prepare by diluting Neutralisation buffer 1:10 in your acid elution buffer (i.e. sample matrix buffer). Example: Mix 1 mL Neutralisation buffer with 9 mL elution buffer. Vortex.
- **PBS-Tween (PBS-T) buffer.** Dissolve 1 Wash tablet in 500 mL ultra pure water. Store prepared PBS-T buffer at + 4°C but not for more than 3 days.
- **Biotinylated anti-SpA IgY Concentrate.** Dilute 1:100 in PBS-T buffer. The solution is not stable for more than 24 hours. Example: Mix 120 µL Biotinylated anti-SpA IgY Concentrate with 12 mL PBS-T buffer. Vortex.
- **HRP conjugate Concentrate.** Dilute 1:100 in PBS-T buffer. The solution is not stable for more than 24 hours. Example: Mix 120 µL HRP conjugate Concentrate with 12 mL PBS-T buffer. Vortex.

## 7. Sample and standard preparation

After reagent preparation, the samples and standard references are prepared before the assay is performed. The steps for sample preparation and test procedure are also summarised in the Quick Start Guides on pages 18 and 19.

### 7.1 Preparing samples (samples with and without IgG):

**Neutral samples:** SpA easily binds to glass and plastic material. However, in the presence of 0.05% Tween 20 this binding is inhibited. In order to avoid this, add Tween solution, 1:400, to the sample tubes *before* adding sample. Next, add sample and mix well. Example: For 2 mL sample volume, add 5  $\mu$ L Tween solution.

**Acidic samples:** Samples should be neutralised to improve the specific immunological detection of SpA. Determine the elution volume of your acid eluted samples. Add 1/10 volume of Neutralisation buffer to each sample (dilution factor: 0.9). Example: Add 100  $\mu$ L Neutralisation buffer to 0.9 mL sample volume. Measure the pH and add Neutralisation buffer until neutral pH is reached. Note the volume of buffer added in order to calculate dilution factor.

### 7.2 Preparing samples (only for samples with IgG):

7.2.1 Determine the IgG concentration in your samples by measuring the optical density at 280 nm ( $OD_{280}$ ). Divide the  $OD_{280}$  value with 1.36 to get the concentration.

7.2.2 Dilute the samples with Dilution buffer so that all samples contain the same IgG concentration (note the volume of buffer added in order to calculate dilution factor).

7.2.3 Transfer 500  $\mu$ L of each sample with adjusted IgG concentration to a labelled Eppendorf tube (not provided).



### 7.3 Preparing Solution G (only for samples with IgG):

7.3.1 Determine the concentration of a SpA-free IgG solution (see 7.2.1).

7.3.2 Add the IgG solution to Dilution buffer in a 10-mL tube (not provided). Example: Add the IgG solution to 5 mL Dilution buffer (approximately 4 mL is needed to prepare standards I, II and III). Adjust the IgG concentration in Solution G to the same as in the samples (see 7.2.2).

### 7.4 Preparing standard references:

7.4.1 Label four Eppendorf tubes from I to IV and prepare the standards as indicated below.

		Samples w/o IgG	Samples with IgG	
Std	Source solution	PBS-Tween	Solution G	SpA conc. (ng/mL)
I	40 $\mu$ L Protein A ref.	760 $\mu$ L <sup>1</sup>	760 $\mu$ L <sup>1</sup>	25000 <sup>1</sup>
II	40 $\mu$ L Std I	960 $\mu$ L	960 $\mu$ L	1000
III	200 $\mu$ L Std II	800 $\mu$ L	800 $\mu$ L	200
IV	100 $\mu$ L Std III	900 $\mu$ L	See step 7.5	20

### 7.5 Removal of IgG (only for samples with IgG):

7.5.1 Make a hole in the cap of the Eppendorf tubes. Place your samples and Standard III (200 ng/mL) in a rack or floating aid and boil in a water bath for 4 minutes. Remove from the water bath and let cool for 5-10 minutes at room temperature.

7.5.2 Centrifuge the boiled tubes at 2000g for 60 seconds.

7.5.3 Add 100 $\mu$ L of the supernatant of your boiled samples and Standard III into 900 $\mu$ L of Dilution Buffer. This gives Standard IV at 20 ng/mL.

Note: This dilution of samples and standards after boiling can be omitted. For more information see section 11, Tips and Hints.

---

<sup>1</sup> The concentration of the reference is 0.5mg/mL (range 0.45 - 0.55mg/ml). For information on more exact preparation of standards, see section 11, Tips and Hints.


## 8. Test procedure

### 8.1 Performing the assay:

8.1.1 Add 100 $\mu$ L of PBS-Tween for samples WITHOUT IgG or Dilution Buffer for samples WITH IgG into row B to H for wells allocated for the standard references.

8.1.2 Add 200  $\mu$ L of Standard IV to wells in row A. It is recommended to test standard references in duplicate. Dilute the standard in the ELISA plate according to figure 1.

**Figure 1.** 1:2 dilutions of Standard IV in the ELISA plate

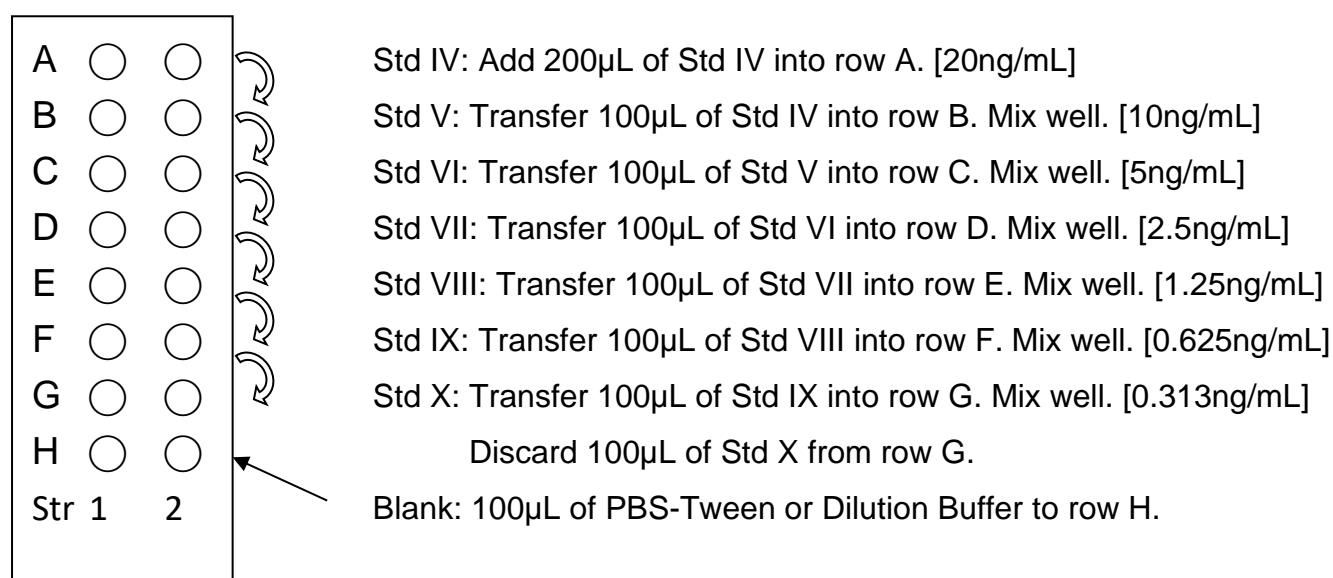

8.1.3 Add 100  $\mu$ L of samples to appropriate wells. It is recommended to test samples in duplicate.

8.1.4 Cover with plastic wrap or tape and incubate the plate for 60 minutes ( $\pm$  6 minutes) at room temperature.

8.1.5 Wash the strips by emptying the wells and then rinsing 4 times with PBS-T buffer, filling all wells to the top for each rinse. Empty the wells by tapping the plate upside down onto a paper towel to remove the last traces of fluid.

- 8.1.6 Add 100  $\mu$ L Biotinylated anti-SpA IgY (diluted) to each well. Cover with plastic wrap or tape and incubate the plate for 60 minutes ( $\pm$  6 minutes) at room temperature.
- 8.1.7 Wash the strips (see step 8.1.5). Add 100  $\mu$ L HRP conjugate (diluted) to each well. Cover with plastic wrap or tape and incubate the plate for 30 minutes ( $\pm$  3 minutes) at room temperature.
- 8.1.8 Wash the strips (see step 8.1.5). Add 100  $\mu$ L Substrate solution to each well and incubate the plate 10 minutes ( $\pm$  1 minute) at room temperature in the dark. Begin timing after the first well is filled.
- 8.1.9 Stop the reaction by adding 100  $\mu$ L Stop solution to each well. Add the Stop solution in the same order as the Substrate solution was added.
- 8.1.10 Measure the absorbance of the samples and standard references at 450 nm within 30 minutes after adding the Stop solution.

## 9. Analysis of results

To determine the exact SpA concentrations in your samples, use data reduction software to automatically generate an appropriate standard curve such as a four-parameter curve fit. Most ELISA reader software programs can correct for background automatically, so consult the user's manual for your specific software.

### 9.1 Manually estimating SpA sample concentration

**Standard curve**: Calculate the mean for the standard reference duplicates and correct for background by subtracting the mean absorbance value for the blank. Plot Corrected OD<sub>450</sub> vs. Concentration on a semi-log paper.

$$\text{OD}_{450} (\text{Standard IV to X}) - \text{OD}_{450} (\text{PBS-Tween or Dilution Buffer}) \\ = \text{Corrected OD}_{450}$$

**Samples**: Calculate the mean absorbance value for the sample duplicates and correct for background by subtracting the mean absorbance value for the blank.

From the corrected OD values, approximate the sample concentration ( $C_S$ ) from the standard curve. To calculate the final SpA concentration ( $C_F$ ) in each of the samples, divide  $C_S$  by the final dilution factor (DF) for each sample. When a sample has been diluted several times, i.e. with neutralisation buffer and then dilution buffer, multiply the dilution factors to get the final dilution factor


$$\text{Final SpA concentration (ng/mL): } C_F = C_S / DF$$

## 10. Performance

The kit has been validated according to general guidelines. An excerpt of results is shown below. The performance information should only be taken as guidance. For quality control purposes, the assay should be validated in-house with respect to common parameters. In the shown results we have used recombinant SpA from GE Healthcare and human IgG (mix of subclasses, primarily IgG<sub>1</sub> och IgG<sub>2</sub>).

### 10.1 Validity of assay

For samples without IgG, Standard IX (0.625 ng/mL) should have a corrected absorbance value greater than 0.1. For samples with IgG, Standard VIII (prepared as 1.25 ppm) should have a corrected absorbance value greater than 0.1.

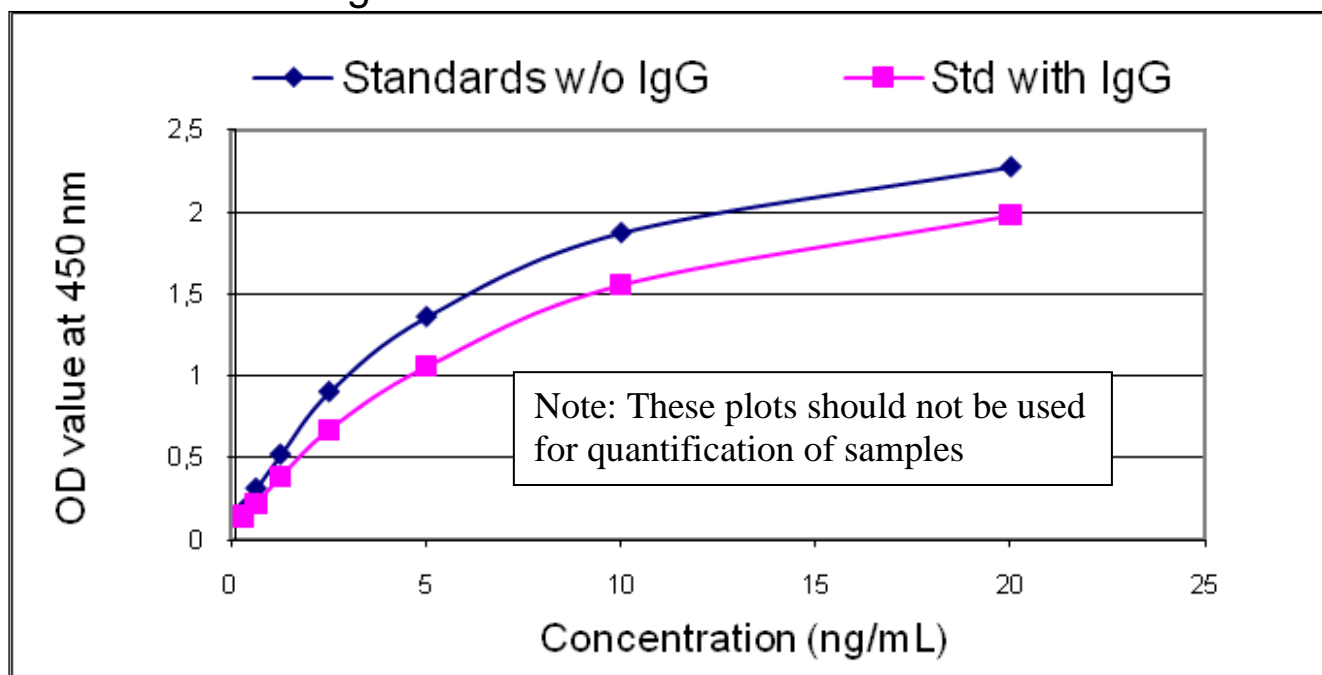

### 10.2 Sensitivity:


The functional sensitivity is 0.15 ng/mL (0.15 ppm<sup>2</sup>). This is set as the concentration where the intra assay CV < 10% and the OD-signal is higher than  $OD_{BLANK} + 3 \cdot SD_{BLANK}$ .

---

<sup>2</sup> The unit parts per million, ppm, is the concentration of Protein A relative to the concentration of IgG, e.g. 1 ng/mL Protein A in 1mg/mL of IgG equals 1 ppm.


### 10.3 Linearity:

The linear range is 0.15 – 33 ng/mL (0.15 – 33 ppm). This is set as the concentration where recovery of standards is 80-120% and a plot of Quantified vs. Theoretical concentration gives  $R^2 > 0.990$ .

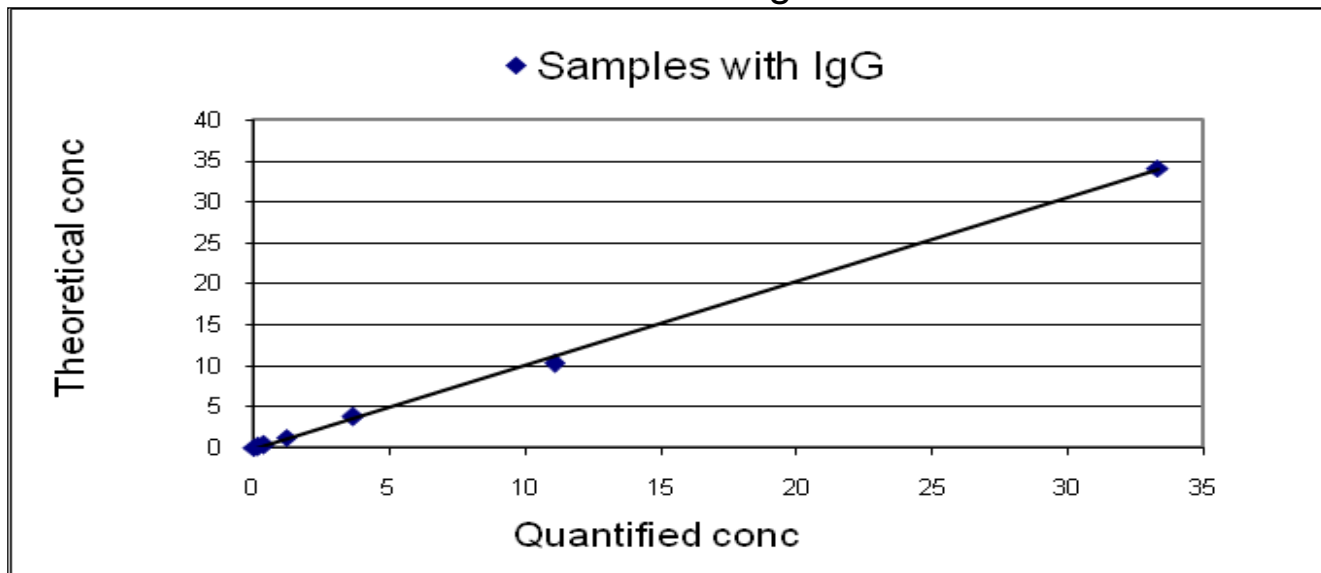

### 10.4 Specificity

Recovery has been tested with different SpA sources, both native and recombinant. Recoveries were in the range 75-150%.

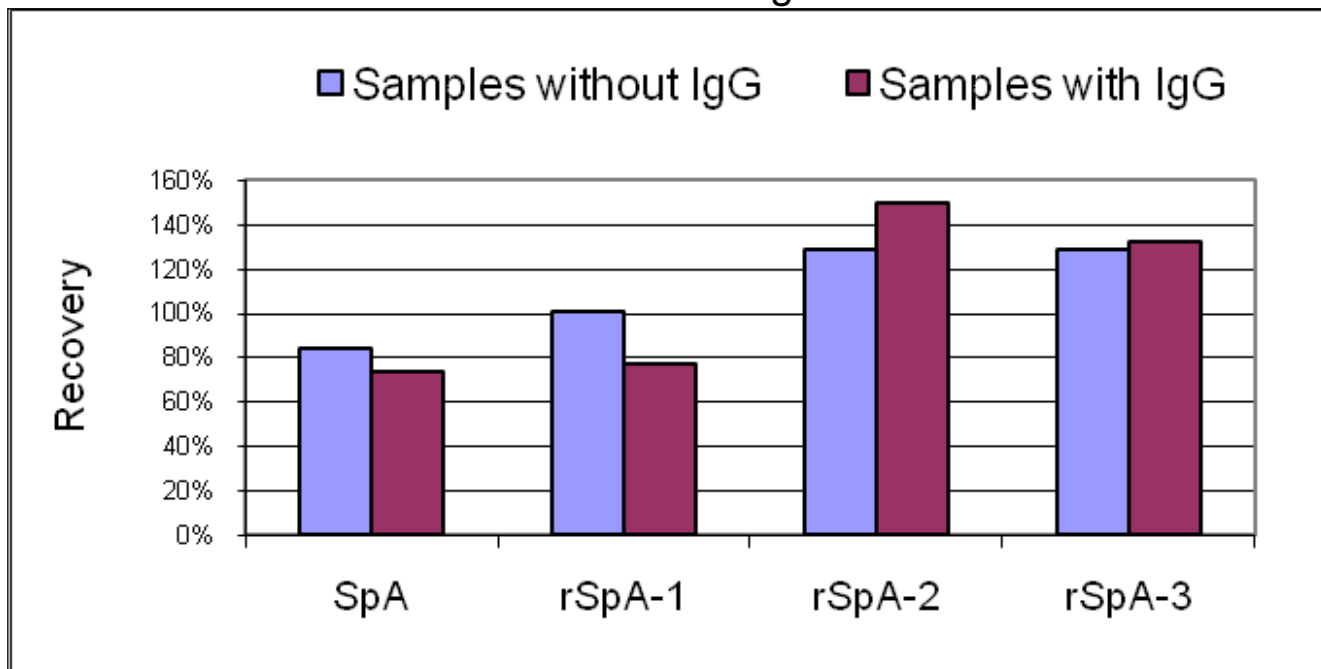

### 10.5 Precision:


Coefficients of variation (CV) for duplicate measurements are typically <10%. The average between-day CV was <15% when tested on 6 different occasions for three samples. The samples were tested in a concentration range 0.5 – 150 ng/mL (ppm).

### 10.6 Recovery:

Samples at three different concentrations were spiked with three different amounts. The recovery was within  $\pm 15\%$  for all samples and amounts spiked.

### 10.7 Matrix effect:

The binding affinity of SpA differs between IgG from different species but also between isotypes of IgG from the same species. Thus, the accuracy of the results will depend on the IgG that is used for the standards. Even with the same IgG, the graph shows the importance of normalizing the IgG-concentration in samples and standards.

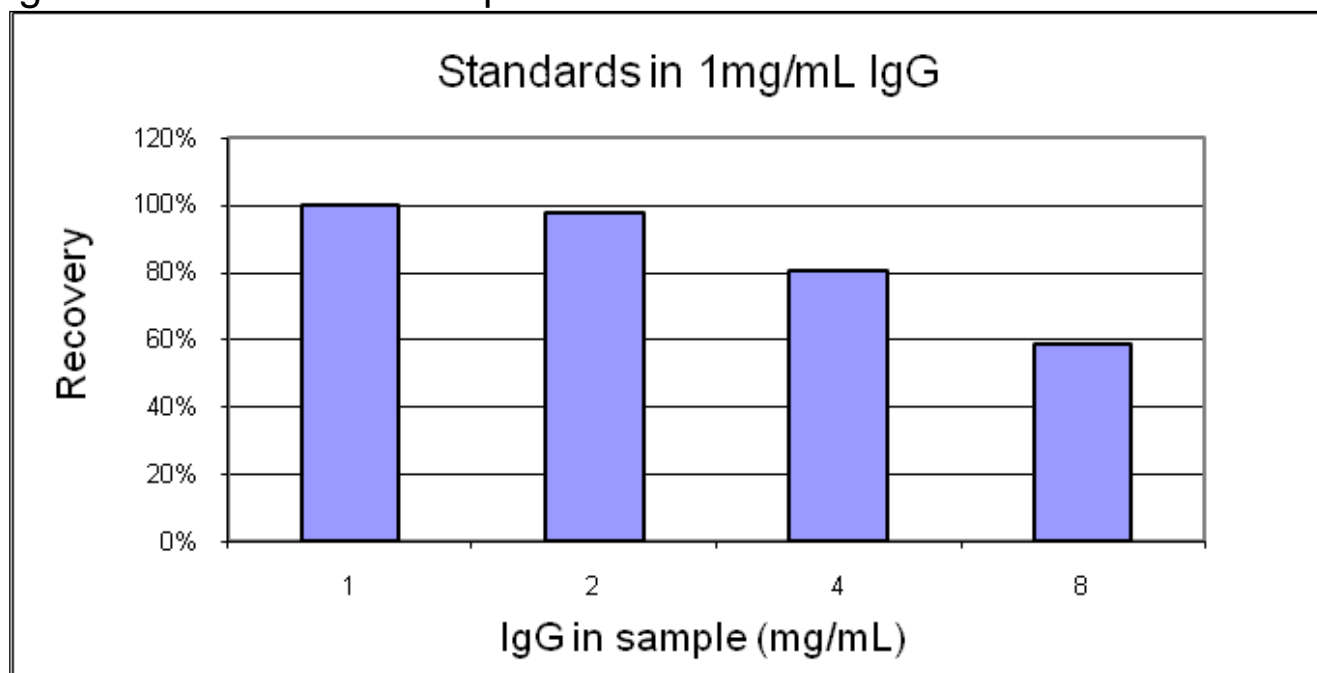

### 10.8 Antigen excess:

No antigen excess effect was seen for standards tested up 1600 ppm.

## 11. Tips and hints

### Preparation of Protein A standards

The concentration of the included Protein A reference is 0.5 mg/mL, i.e. in the range 0.45 - 0.55 mg/mL. A more exact concentration can be retrieved from the Product Certificate for the component. To prepare more exact standards, the volume indicated for Std I in table 7.4.1 should be adjusted to obtain a concentration of 25000 ng/mL.

Sample calculation where PrA concentration on certificate is given as 0.53 mg/ml:  $0.53 \text{ mg/mL} * 40 \text{ } \mu\text{L} / 0.025 \text{ mg/mL} = 848 \text{ } \mu\text{L}$ . For preparation of Std I, 808  $\mu\text{L}$  of PBS-Tween (or Solution G) should be used.

### Dilution of standards and samples for samples with IgG

The 1:10 dilution of standards and samples that is performed after boiling of samples can be omitted. This may be desired if a ten-fold dilution of samples makes them too diluted. In this case, Standard III in the table (section 7.4) should be further diluted 1:10 in solution G, giving Standard IV at 20 ng/mL. Do not mix these two procedures! It is important to keep the same exact procedure for samples and standards.

## 12. Related products

### MouSelect

#### Product number: 09-04

The MouSelect kit contains the basic components needed to set up a sandwich ELISA for the assessment of Protein A binding. The components are designed to aid in an early selection of polyclonal or monoclonal antibodies, to a preferential purification on Protein A (from *Staphylococcus aureus*). The kit can also be used to optimise the Protein A binding of antibodies.

### anti-Protein A

#### Product number: 01-008


IgY fraction. After purification, the antibodies can be used in various immunological applications to detect Protein A (from *Staphylococcus aureus*).




## 13. References

- Forsgren A. et al., SpA and its exploitation. In: Staphylococci and Staphylococcal infections 2 (Eds. C.S.F. Easmon and C. Adlam), pp. 429-480, Academic Press Inc., London (1983).
- Lindmark R. et al., Binding of immunoglobulins to SpA and immunoglobulin levels in mammalian sera. J. Immunol. Methods, 62, 1-13 (1983).
- Langone J.J. et al., Radioimmunoassays for SpA of Staphylococcus aureus. J. Immunol. Methods, 63, 145-157 (1983).
- Berglund A. et al., G01N 33/563 G01N 33/569; Ways to determine Fc-binding bacterial polypeptides. The Swedish Patent Administration, Edition number, 448 190 (1987).
- Larsson A. et al., A microELISA useful for determination of SpA-binding monoclonal antibodies. Hybridoma, 9, 289-294 (1990).

## 14. Quick start guide, samples without IgG

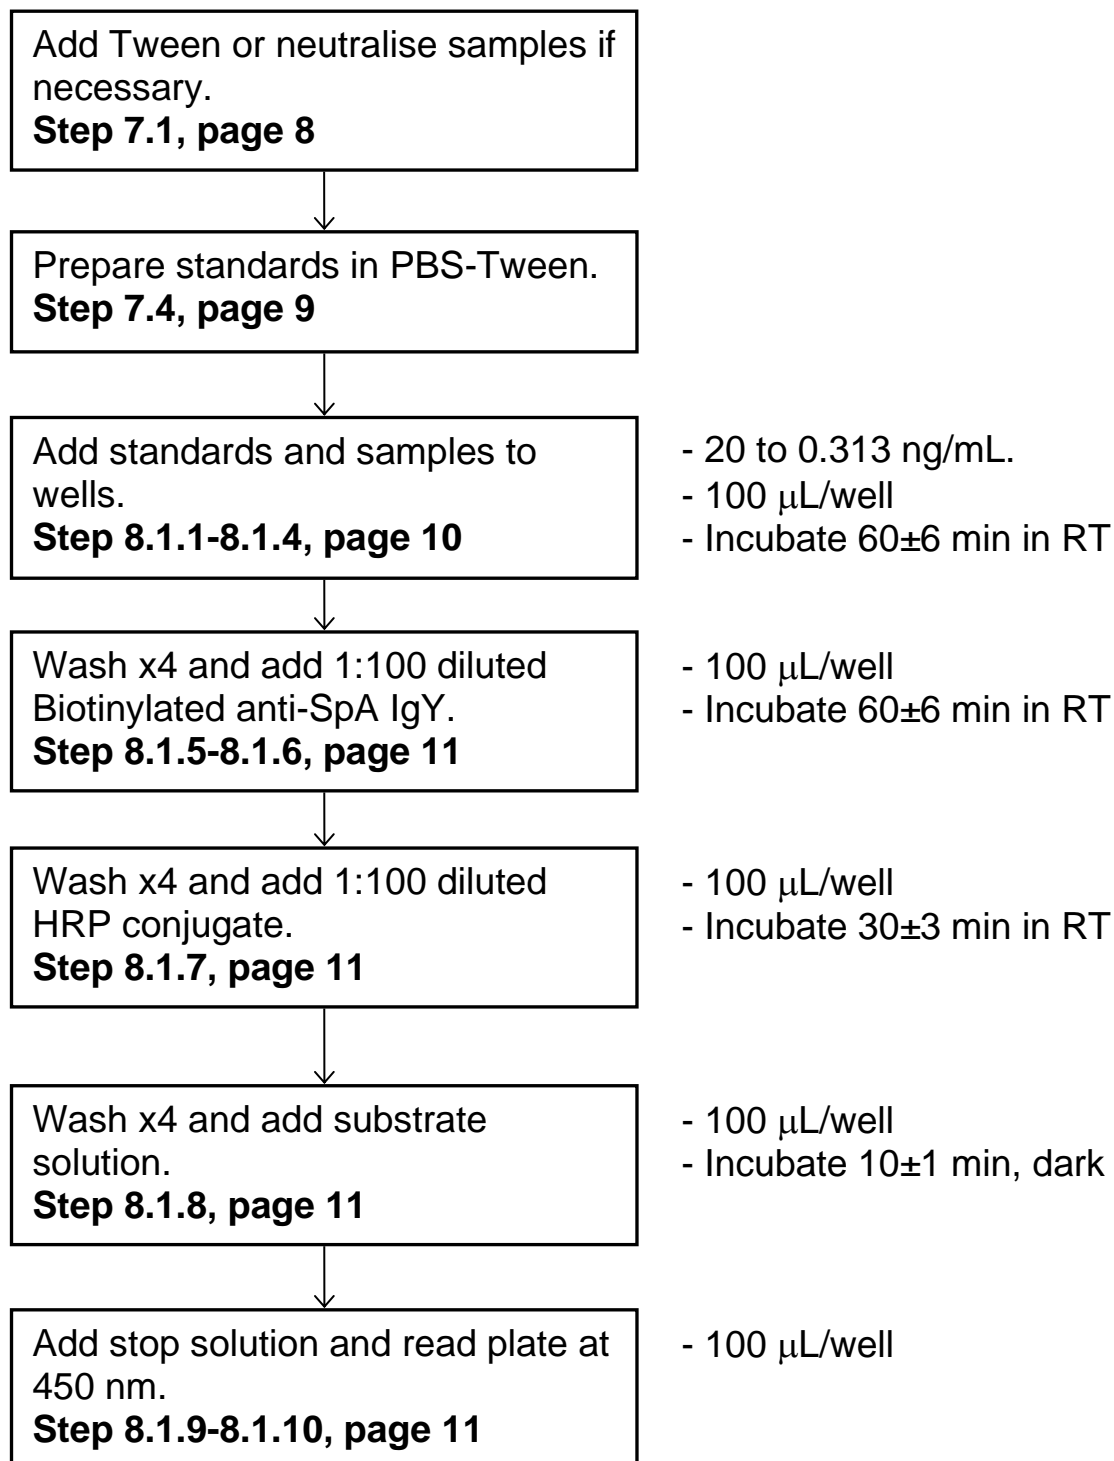

## 15. Quick start guide, samples with IgG

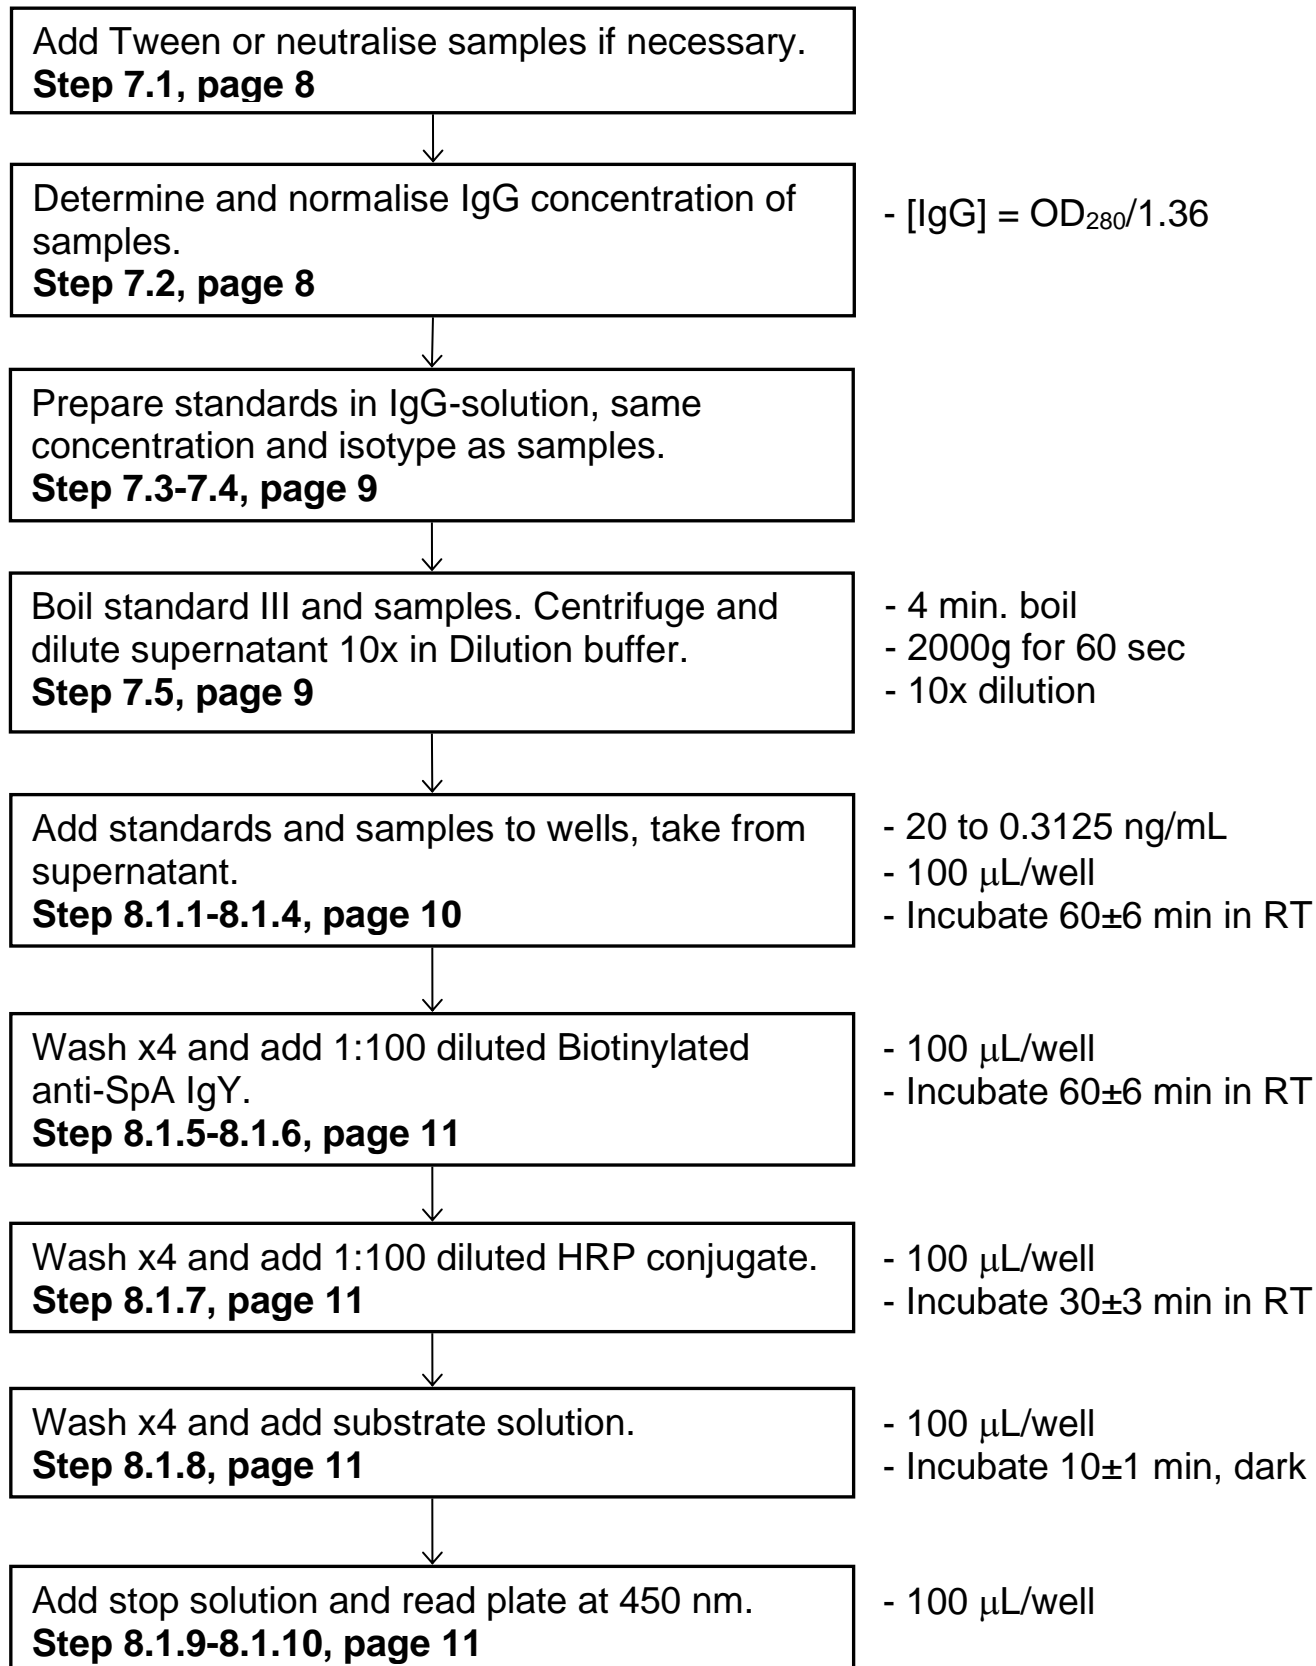

## **16. Contact and order information**

IgY Lab Systems AB  
Boksta 505  
S-744 95 Vittinge, Sweden  
[info@igylabs.com](mailto:info@igylabs.com)

Please visit [www.igylabs.com](http://www.igylabs.com) for additional information.

